

Temperature monitoring in bottles with SterilDisk Can

1- If you can fix the crown cap AFTER having fixed the logger, you can use:


A- Copunterbolt, screwed on the threaded part of the probe



B – Locking nut, to adjust depth (point must stay 2 cm from the bottom)



Possibilities:

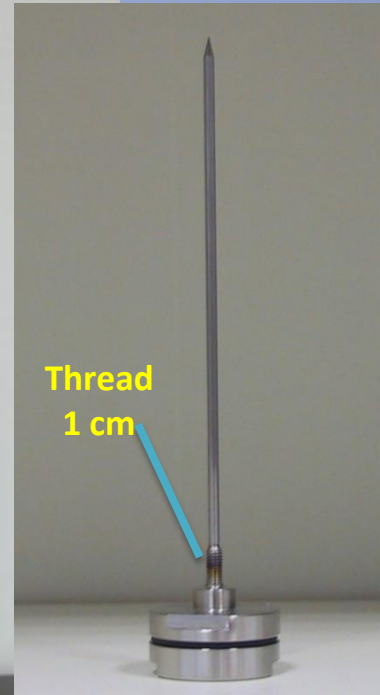

2- If you cannot fix the crown cap AFTER having fixed the logger on it, use the the fitting systems to fix a threaded rivet on the cap and then screw on it the probe

